



3.4 Cleaning the instrument

Remove the buffer

1. Lift the instrument cover.
2. Remove the cartridge and dispose of it in a bio-hazardous waste container.
3. Insert the cleaning cartridge and clamp in place.
4. Empty the ice container.
5. Attach the buffer extension tubing to the buffer outlet located in the buffer reservoir. Place the other end into a bucket (below instrument level) or a nearby sink.

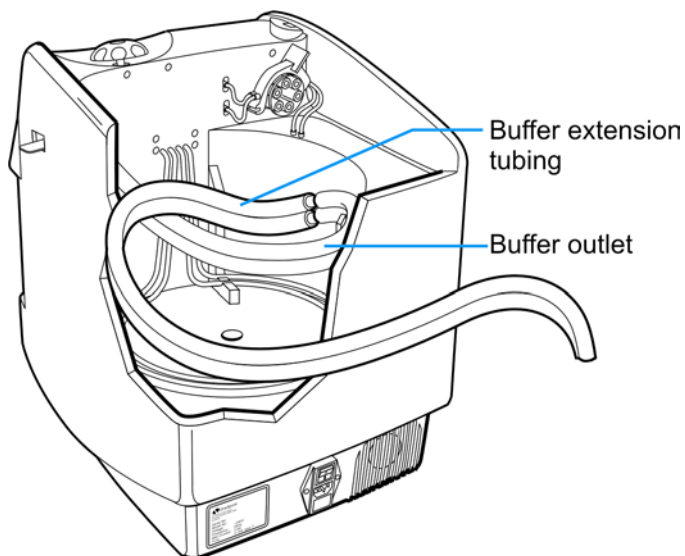

6. Press the  button to empty the buffer reservoir.